

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
9 June 2005 (09.06.2005)

PCT

(10) International Publication Number
WO 2005/051469 A1

(51) International Patent Classification⁷: **A61M 16/00**

[AU/AU]; ResMed Limited, 97 Waterloo Road, North Ryde, New South Wales 2113 (AU).

(21) International Application Number:
PCT/AU2004/001651

(74) Agents: **DAVIDSON, Geoffrey, Robert** et al.; Halford & Co., 1 Market Street, Sydney, New South Wales 2000 (AU).

(22) International Filing Date:
25 November 2004 (25.11.2004)

(81) Designated States (*unless otherwise indicated, for every kind of national protection available*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BW, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EC, EE, EG, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NA, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA, UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
60/525,219 26 November 2003 (26.11.2003) US

(71) Applicant (*for all designated States except US*): **RESMED LIMITED** [AU/AU]; 97 Waterloo Road, North Ryde, New South Wales 2113 (AU).


(84) Designated States (*unless otherwise indicated, for every kind of regional protection available*): ARIPO (BW, GH, GM, KE, LS, MW, MZ, NA, SD, SL, SZ, TZ, UG, ZM, ZW), Eurasian (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),

(72) Inventor; and

(75) Inventor/Applicant (*for US only*): **BASSIN, David, John**

[Continued on next page]

(54) Title: **METHODS AND APPARATUS FOR THE SYSTEMIC CONTROL OF VENTILATORY SUPPORT IN THE PRESENCE OF RESPIRATORY INSUFFICIENCY**

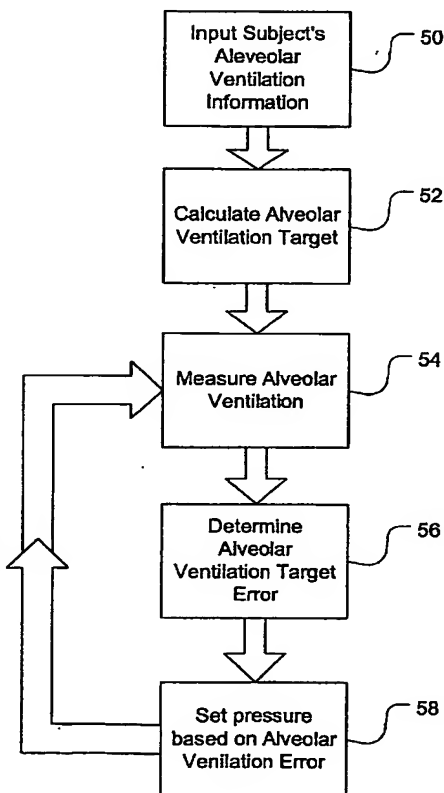

(57) Abstract: A method and apparatus for providing ventilatory assistance to a spontaneously breathing patient. An error signal (56) is computed that is the difference between a function of respiratory airflow (54) over a period of time and a target value (52). Using a servo loop, air is delivered to the patient at a pressure that is a function of the error signal, the phase of the current breathing cycle, and a loop gain that varies depending on the magnitude of the error signal. The loop gain increases with the magnitude of the error signal, and the gain is greater for error signals below a ventilation target than for error signals above the ventilation target value. The target value (52) is an alveolar ventilation that takes into account the patient's physiologic dead space.

WO 2005/051469 A1



European (AT, BE, BG, CH, CY, CZ, DE, DK, EE, ES, FI, FR, GB, GR, HU, IE, IS, IT, LU, MC, NL, PL, PT, RO, SE, SI, SK, TR), OAPI (BF, BJ, CF, CG, CI, CM, GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

Published:

— *with international search report*